

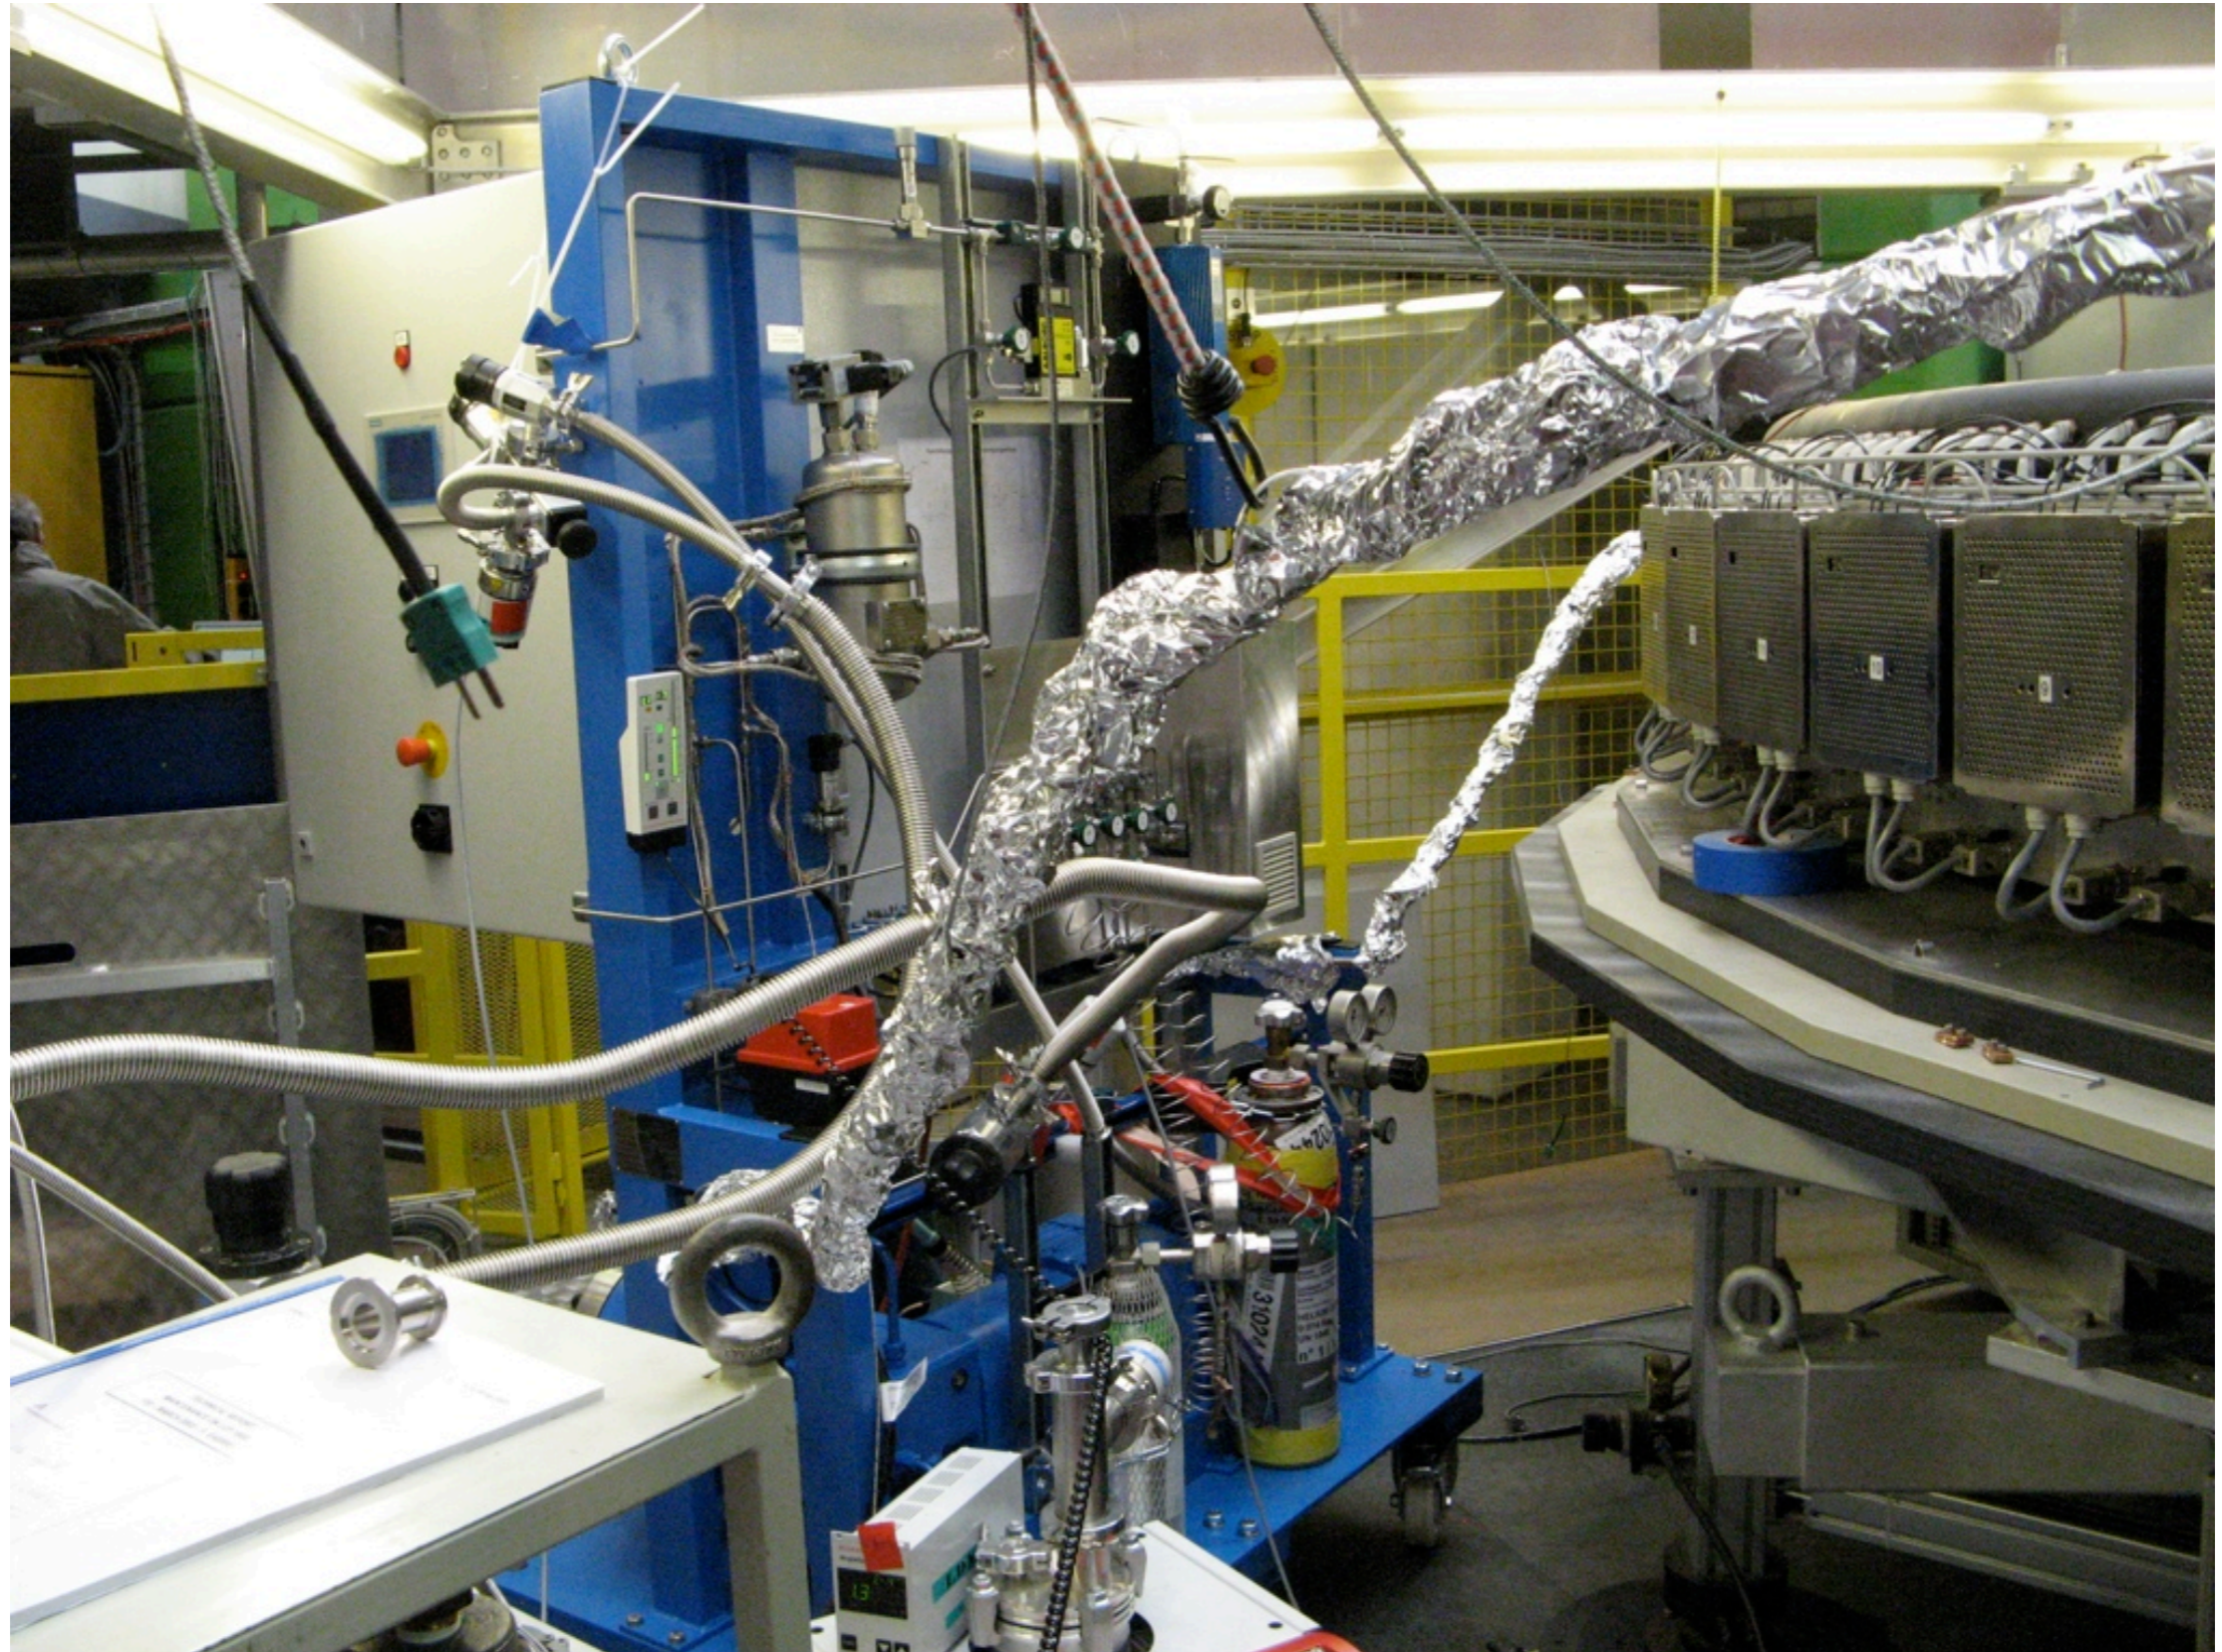


View of the HRPT gas mixture cleaning/adding system

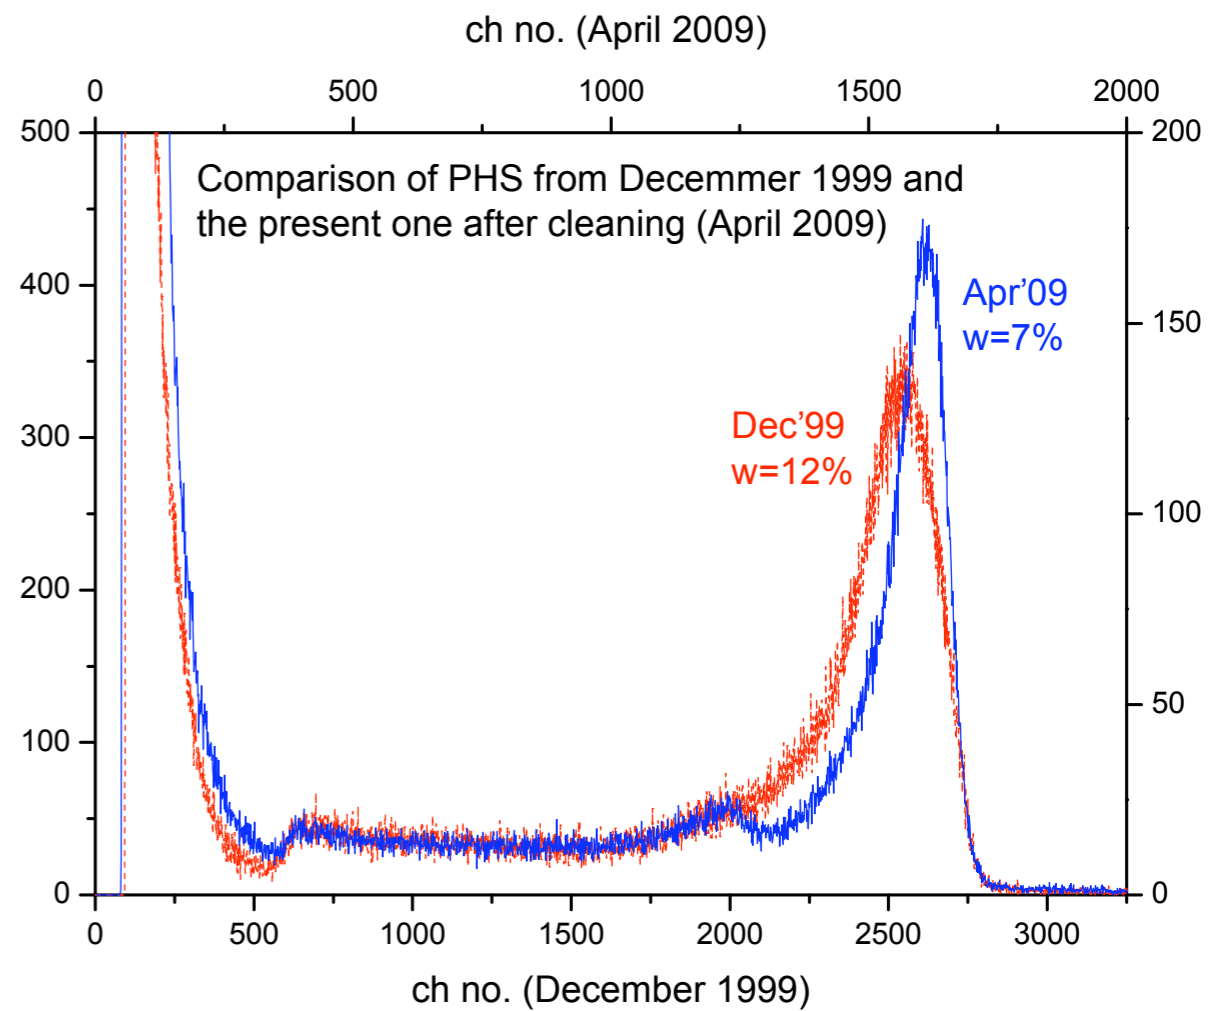

Comparison of the Pulse Height Spectra before (2008) and after (2009) HRPT gas cleaning/pressurizing

HRPT PHS, monodetector 1.6kV.
Am-Be n-source. March'09

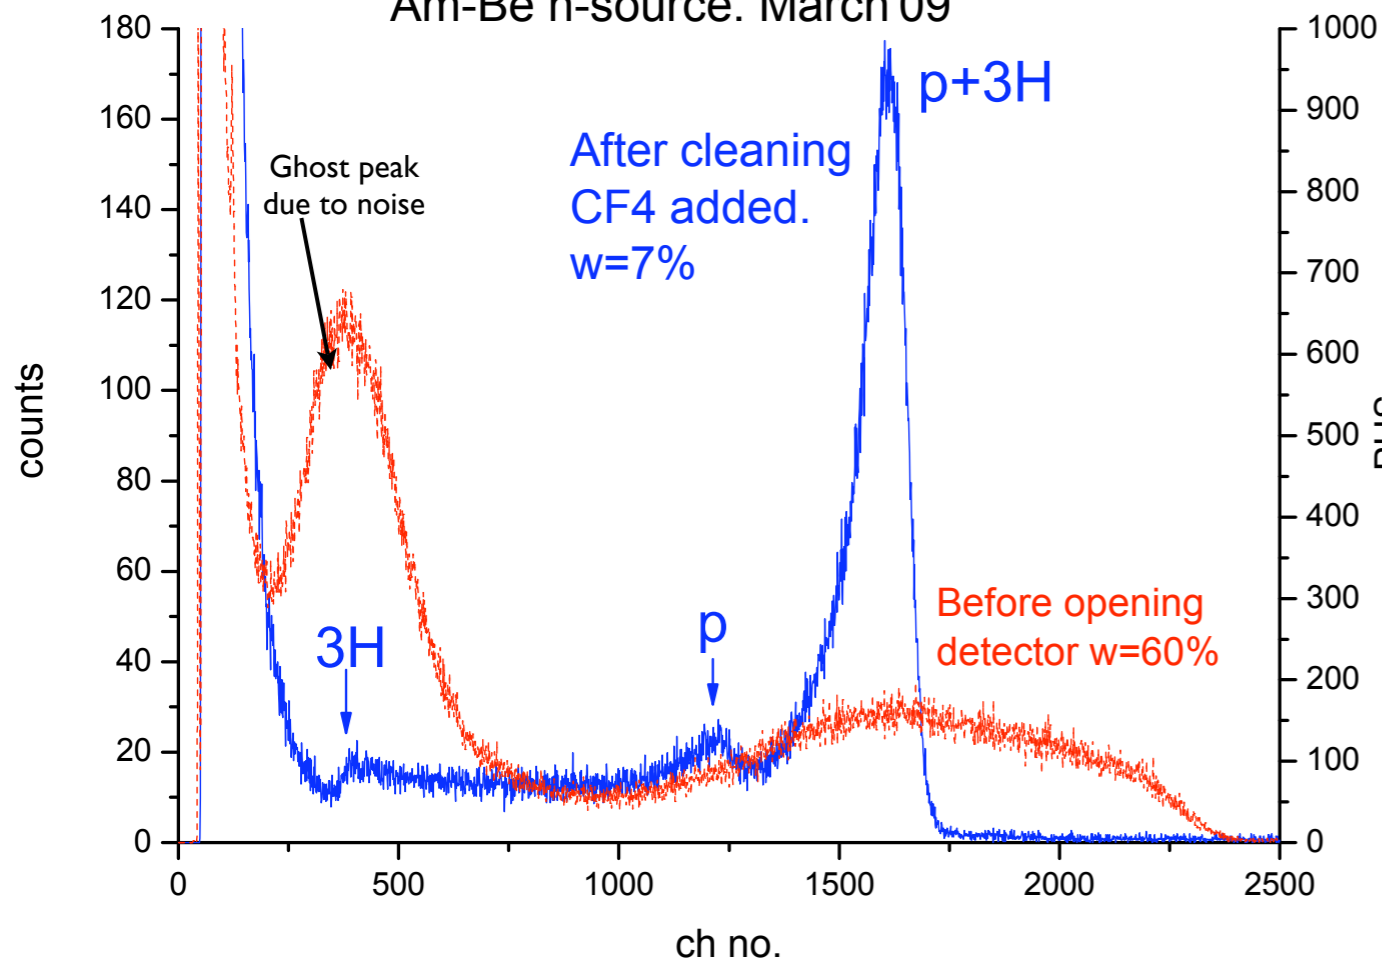

Comparison of the diffraction patterns before (2008) and after (2009) HRPT gas cleaning/pressurizing

NAC,1.8857,HI,a4=5.0 Sample='NAC'
Monitor 29500000 WaveLength 1.8857

nac8_1p9hi_2009_carusel.dat,nac8_1p9hi_2008_carusel.dat

